INVITATION TO BID

State of Ohio
Department of Administrative Services
General Services Division
Office of Procurement Services

The Original Signed Bid must be submitted to the Office of Procurement Services to receive consideration for award.	BIDDER NAME
BID NUMBER: OT900116 / OPENING DATE (1:00 p.m.): May 13, 2015	STREET ADDRESS ☐ Check if remit address is different and list on separate sheet
	CITY / STATE / ZIP
General Services Division Office of Procurement Services 4200 Surface Road Columbus, OH 43228-1395 Attn: Bid Desk	COUNTY / MBE/EDGE CERTIFICATE NUMBER
	TELEPHONE NO. ( ) / TOLL FREE NO. 1 - ( )
	CONTACT PERSON / FAX NO. ( )
REQ./INDEX NO. DRC009 / BID NOTICE DATE 5/5/15	CONTRACTOR'S E-MAIL ADDRESS

SELECT YOUR PREFERRED METHOD OF RECEIVING PURCHASE ORDERS AND ENTER THE E-MAIL OR FAX NUMBER INFORMATION (ONLY SELECT ONE METHOD)

☐ E-Mail ☐ Fax

In addition to the standard terms for payment, the payment terms for state agency(ies) will be 2%,10 Days, Net 30 Days unless otherwise stated in the following space. If no discount is offered, bidder should circle "Net 30 Days". _____%, ____Days, Net 30 Days

PARTICIPATING AGENCY(IES):

OHIO DEPARTMENT OF REHABILITATION AND CORRECTION, FRANKLIN MEDICAL CENTER, 1890 HARMON AVE, COLUMBUS, OHIO 43223

ADDENDUM FOR CHANGE
ADDENDUM NO.: 1
REVISION DATE: 05/05/15

THE DEPARTMENT OF ADMINISTRATIVE SERVICES, OFFICE OF PROCUREMENT SERVICES IS SOLICITING BIDS FOR:

MAGNETIC RESONANCE IMAGING (MRI) SYSTEM PURCHASE/RENTAL AND SERVICE

As indicated herein this addendum is issued to display questions from the Site Visit.

Questions and Answers from Site Visit

1.	Q. What is the height clearance of the Gate?	A. 166 inches
2.	Q. What is the Electrical connection?	A. 200 amp breaker box with 3 phase
3.	Q. What entry is requested into the MRI system?	A. A lift or ramp and stairs.
4.	Q. Is there city water?	A. Yes
5.	Q. Who supplies the electric?	A. Columbus Power
6.	Q. Is the MRI System on the backup generator?	A. Yes
7.	Q. What kind of data troubleshooting is preferred?	A. Prefer remote diagnostic.
8.	Q. Can pictures of the Electrical box and current unit be provided?	A. Yes, See below.
9.	Q. What is the average daily/yearly usage.	A. See below

Procedure Description	Totals for Rolling Year (August 1, 2013-July 31.2014)	Aug	Sept	Oct	Nov	Dec	Jan	Feb	Mar	Apr	May	Jun	Jul
MRI Upper Ext WO	2		1									1	
MRI Upper Ext W/WO	5			1		1				2	1		
MRI Upr Ext Jnt WO	18	2	2	3		1	5	2		2		1	
MRI Upr Ext Jnt w/WO	9	2	1		1	1				2	1	1	
MRI Upr Ext Jnt W	2		1		1								
MRI THR Spn WO	7	1	1	1			1			1		1	1
MRI THR Spn W	8	1	1	1						1	1	1	2
MRI THR Spn W/WO	1							1					
MRI Pelvis WO	1											1	
MRI Pelvis W/WO	11			1	3	2	1	2		1	1		
MRI Orbits WO	1							1					
MRI Orbits W/WO	9		2	2			1	1		1	1	1	
MRI Neck and Spine W/WO	6	1	1				1	2				1	
MRI Lwr Jnt WO	24	3	1		4	4	2				7	3	
MRI Lwr Jnt W/WO	9			2			2			2	1	2	
MRI Lwr Jnt W	3											3	
MRI Lwr Ext WO	8					1	1	1	1		1	2	1
MRI Lwr Ext W/WO	11	3						2	1	4	1		
MRI Lmbr Spn WO	26	1	4		3	2	1	1	5	2	4	2	1
MRI Lmbr Spn W/WO	18	1	1	2	2	2				3	3	1	3
MRI Crv Spn WO	30	3	5	3	1	2	3	3		2	1	4	3
MRI Crv Spn W	20	2	4	4		1	2	1			2	1	3
MRI Crv Spn W/WO	1									1			
MRI Chest and Spn WO	1						1						
MRI Brain WO	13	2	1				1	3		1	5		
MRI Brain W/WO	88	7	7	11	5	6	7	8	3	9	6	10	9
MRI Abd WO	1					1							
MRI Abd W/WO	27	2	2	1	2	4	5	3	2	2	3	1	
MRI Abd W	1			1									
MRA Head and Neck W/WO	1												1
MRCP	2			1								1	
MRA Neck W/O	2	1						1					
MRA Head W/O	8	1		1				2			1		3
MRA Head W/WO	2				1					1			
MRA Head W	1									1			
Total Scans for Rolling Year	377	33	35	35	23	28	34	34	12	38	40	38	27

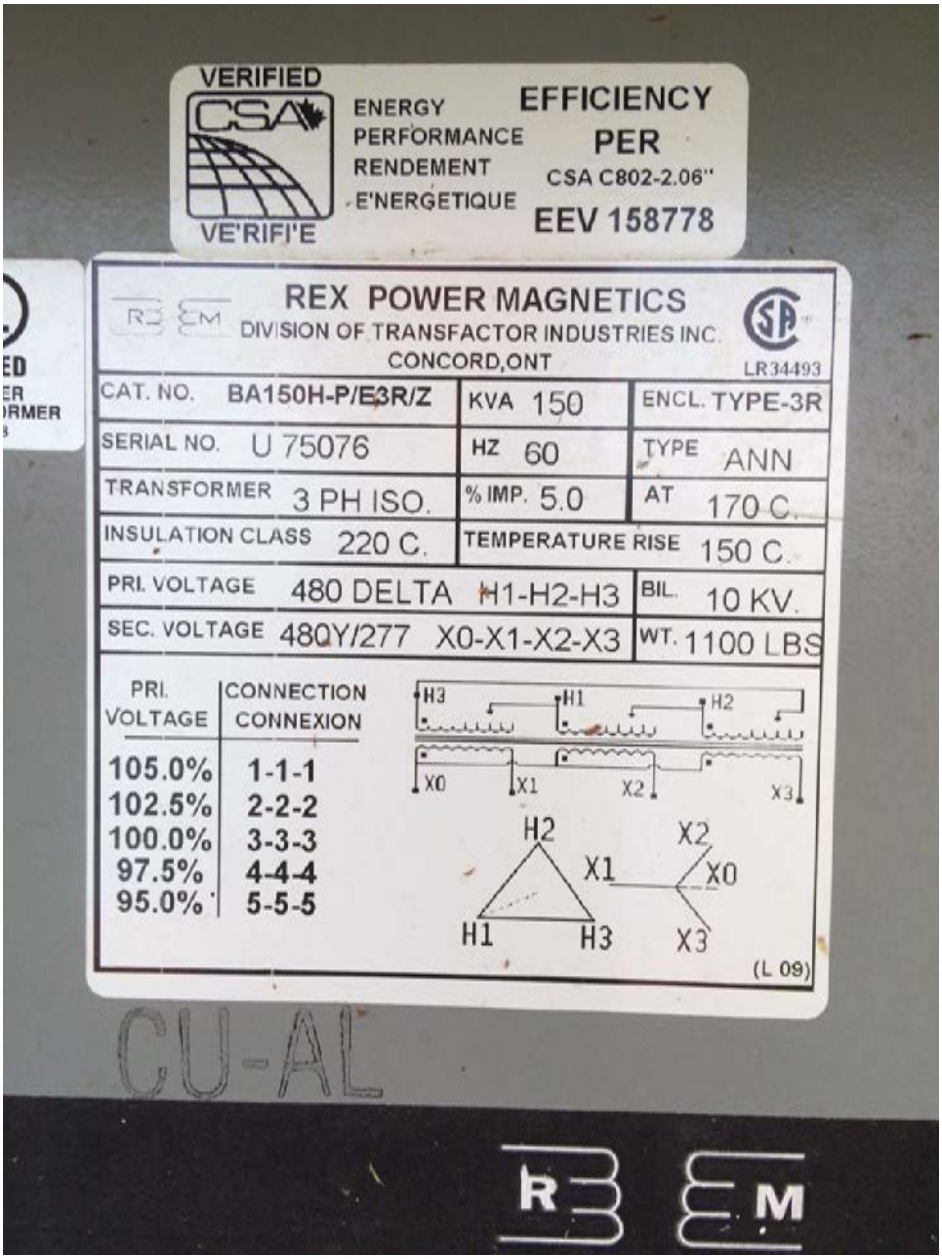
VERIFIED
CSA
VE'RIFI'E
ENERGY
PERFORMANCE
RENDEMENT
E'NERGETIQUE
EFFICIENCY
PER
CSA C802-2.06"
EEV 158778
REX POWER MAGNETICS
DIVISION OF TRANSFACTOR INDUSTRIES INC.
CONCORD,ONT
LR34493
CAT. NO. BA150H-P/E3R/Z
KVA 150
ENCL. TYPE-3R
SERIAL NO. U 75076
HZ 60
TYPE ANN
TRANSFORMER 3 PH ISO.
% IMP. 5.0
AT 170 C.
INSULATION CLASS 220 C.
TEMPERATURE RISE 150 C.
PRI. VOLTAGE 480 DELTA H1-H2-H3
BIL. 10 KV.
SEC. VOLTAGE 480Y/277 X0-X1-X2-X3
WT. 1100 LBS
PRI. VOLTAGE
CONNECTION CONNEXION
105.0% 1-1-1
102.5% 2-2-2
100.0% 3-3-3
97.5% 4-4-4
95.0% 5-5-5
H3
H1
H2
X0
X1
X2
X3
H2
X1
H1
H3
X2
X0
X3
(L 09)
CU-AL
R
M

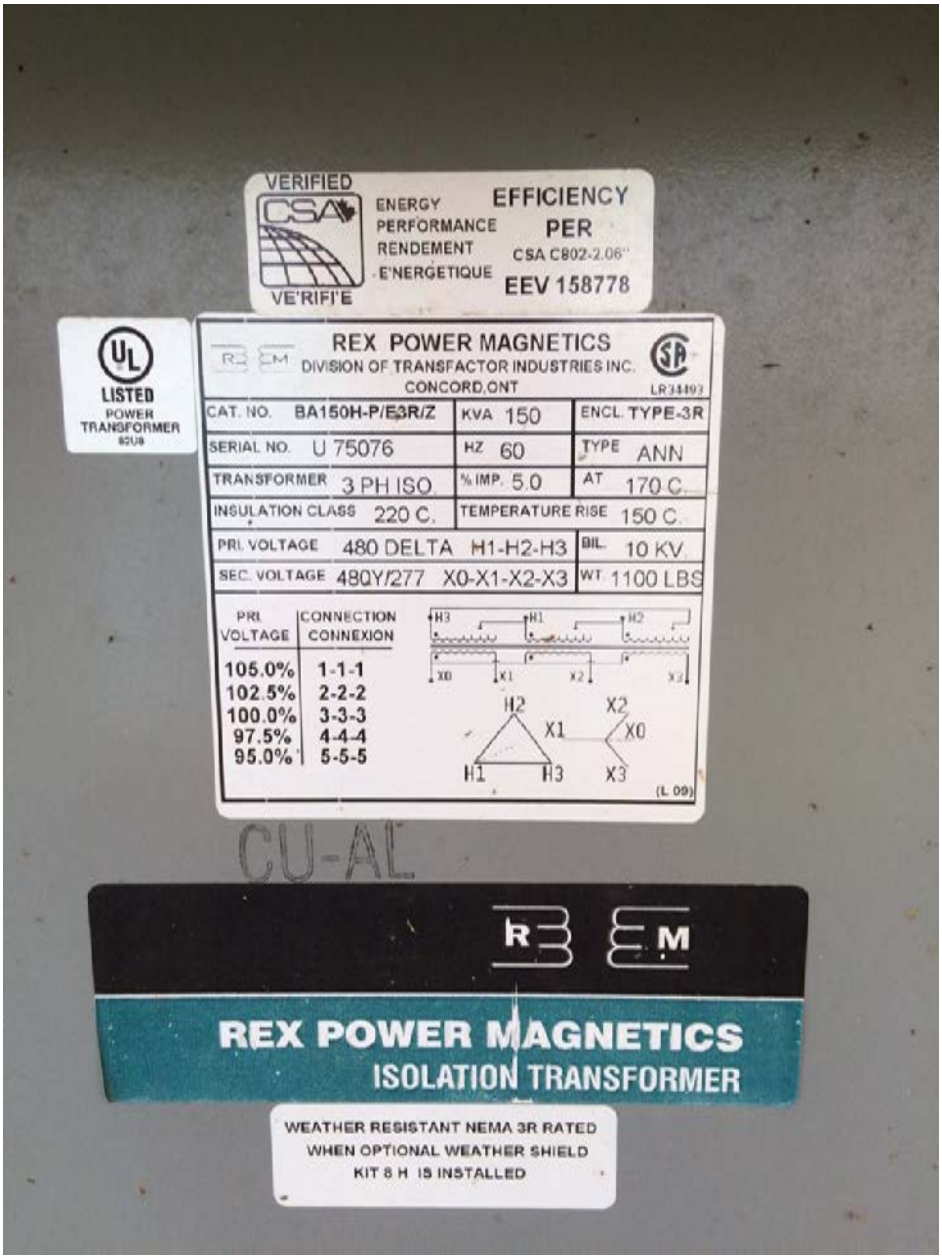
VERIFIED
CSA
VE'RIFI'E
ENERGY
PERFORMANCE
RENDEMENT
E'NERGETIQUE
EFFICIENCY
PER
CSA C802-2.06
EEV 158778
LISTED
POWER
TRANSFORMER
REX POWER MAGNETICS
DIVISION OF TRANSFACTOR INDUSTRIES INC.
CONCORD,ONT
LR34493
CAT. NO. BA150H-P/E3R/Z
KVA 150
ENCL. TYPE-3R
SERIAL NO. U 75076
HZ 60
TYPE ANN
TRANSFORMER 3 PH ISO.
% IMP. 5.0
AT 170 C.
INSULATION CLASS 220 C.
TEMPERATURE RISE 150 C.
PRI. VOLTAGE 480 DELTA H1-H2-H3
BIL 10 KV.
SEC. VOLTAGE 480Y/277 X0-X1-X2-X3
WT. 1100 LBS
PRI. VOLTAGE
CONNECTION CONNEXION
105.0% 1-1-1
102.5% 2-2-2
100.0% 3-3-3
97.5% 4-4-4
95.0% 5-5-5
H3
H1
H2
X0
X1
X2
X3
H2
X1
H1
H3
X2
X0
X3
(L 09)
CU-AL
REX POWER MAGNETICS
ISOLATION TRANSFORMER
WEATHER RESISTANT NEMA 3R RATED
WHEN OPTIONAL WEATHER SHIELD
KIT 8 H IS INSTALLED

SIEMENS
ON
OFF

SIEMENS
WARNING
Potential
Arc Flash
Hazard
ON
OFF

574

SHARED IMAGING
DELIVERING ACCOUNTABLE CARE WITH FLEXIBLE ASSETS
CT, MRI AND PET/CT SYSTEMS